Helping all people live healthy lives

BD SafetyGlide™ Shielding Hypodermic Needle

QUICK REFERENCE CARD

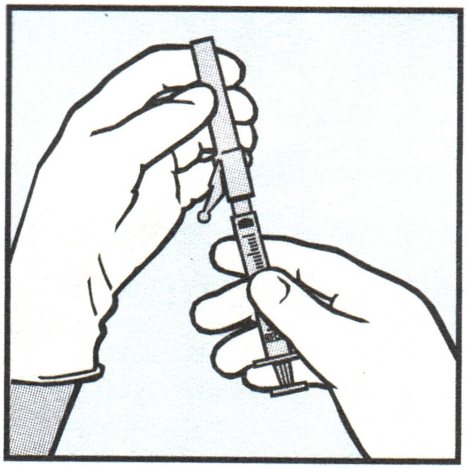

1. Attachment

Attach the BD SafetyGlide™ Needle to any standard BD Luer-Lok™ or luer-slip hypodermic syringe.

Twist until firmly seated.

Pull shield straight off needle to avoid damaging needle point.

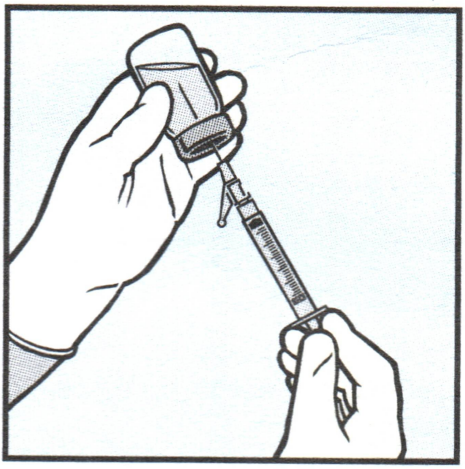

2. Aspiration

Draw up medication in accordance with established protocol.

BD SafetyGlide™ Shielding Hypodermic Needle

QUICK REFERENCE CARD

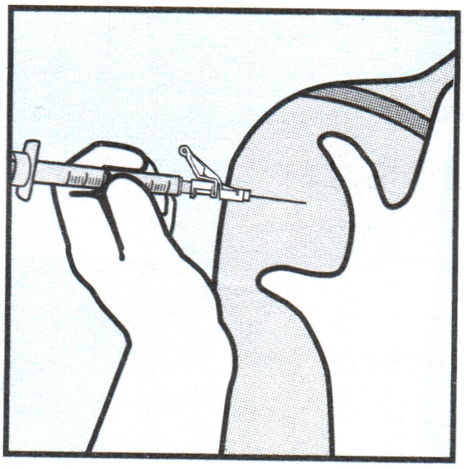

3. Injection

Administer medication in accordance with established protocol.

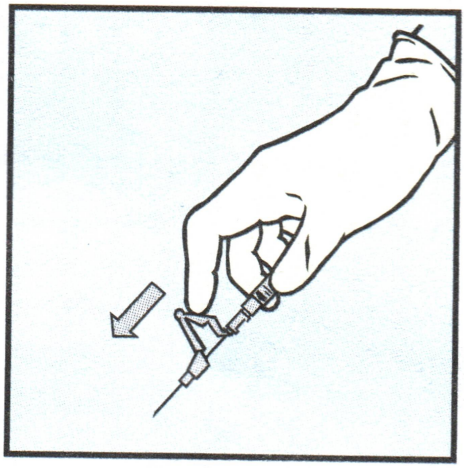

4. Activation

Immediately after injection, and removal from patient activate safety mechanism by pushing the lever arm forward until needle tip is completely covered.
NOTE: Activate away from self and others. Visually confirm needle tip is fully covered

After activation, discard immediately into the nearest sharps container.

Things to Remember:

- When using the BD SafetyGlide™ Needle, be sure to push lever forward with finger to activate safety mechanism.
- Aseptic technique and proper skin preparation of the site are essential.
- Discard the BD SafetyGlide™ Needle and syringe after single use in an approved sharps collector. Follow your institution's policy for safe disposal of all medical waste

BD, BD Logo and all other trademarks are property of Becton, Dickinson and Company. ©2012 BD
1 Becton Drive, Franklin Lakes, NJ 07417 1.888.237.2762 www.bd.com
Printed in USA
BD 10/12-MSS0086